

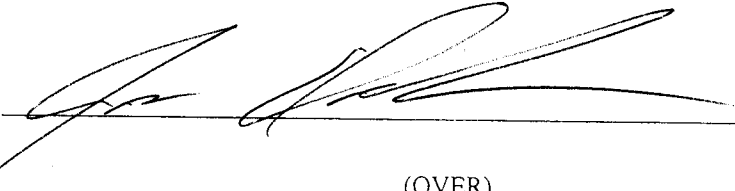
VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

DEC 21 2009

State of Alaska

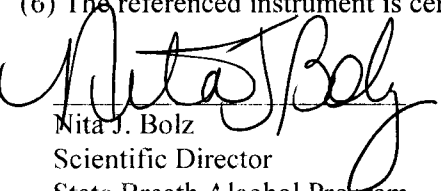
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130297
Name		JAMES HOELSCHER	ID# 5343 Date 12-15-09
A	Agency	AST/VPSO HOOPER BAY	Phone # 758-4615
Instrument Location		Hooper Bay, AK	
Alco S/N		X301526	Target Value .080 High Pressure 600 psi
B	Alco Test Value Average		.081 .081
		1 st Alco	2 nd Alco
Signature			
		(OVER)	

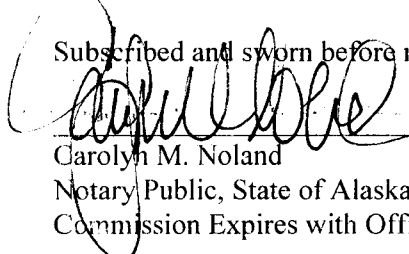
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 8th day of Jan 2010


Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130 297

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130297

DECEMBER 15, 2009

OPERATOR'S NAME: *AMB 1/5/10*
HOELSCHER/JAMES/C
OPERATOR'S NUMBER: 5343
SUBJECT'S LAST NAME:
VERIFICATION
SUBJECT'S FIRST NAME/MI :
OF CALIBRATION

O.L. #: N/A
DEPT/AGENCY: HPB1
CASE/REPORT: N/A
TEST TYPE: V
ALCO TARGET VALUE: .000
ALCO S/N: X301526

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 30.04 in		
ALCO TARGET	.000	12:49
BLANK TEST	.000	12:50
INTERNAL STANDARD	VERIFIED	12:50
ALCO TU 30.04 in	.001	12:50
BLANK TEST	.000	12:51
SUBJECT SAMPLE	.000	12:52
BLANK TEST	.000	12:52
ALCO TU 30.04 in	.001	12:53
BLANK TEST	.000	12:53

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130297

DECEMBER 15, 2009
TIME 12:47

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHANGER: 40c
BREATH TUBE: 42c
BAROMETER: 30.04 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?AB CDEFG
HIJKLM NOPQRSTU VWXYZ[\]^_`abcde fghijklmno
pqrstu vwxyz{|}~